


GMDN Term Assignment Rules

The Same Code. Across the Entire Ecosystem.

Once a GMDN Code enters a registration system, it doesn't stay there. The same GMDN Term travels through procurement, clinical use, post-market surveillance, inventory management and registries, connecting data that was previously siloed.

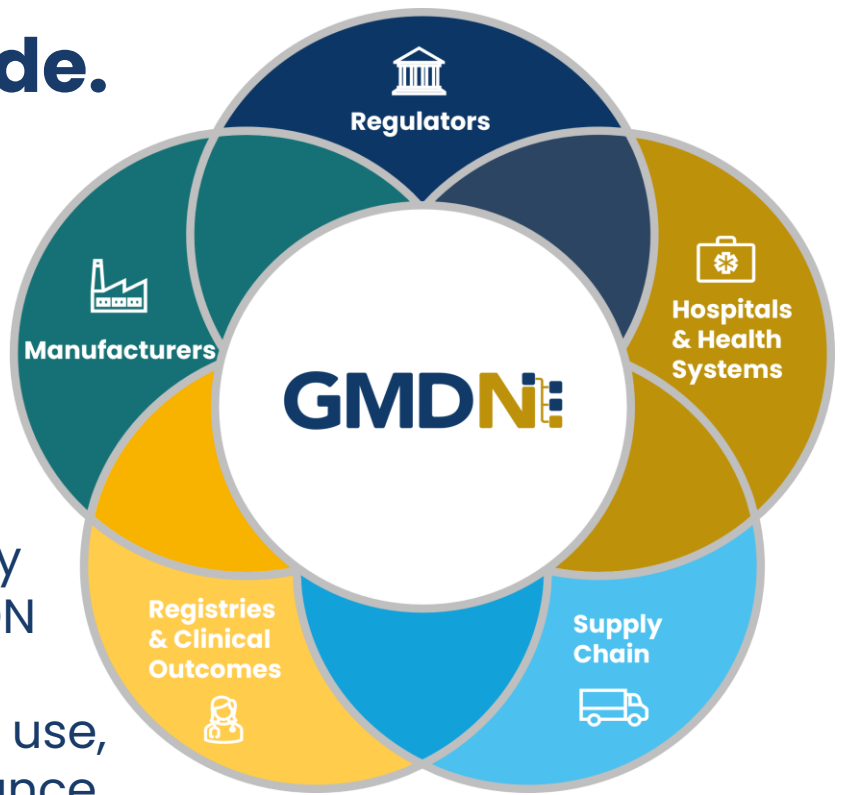

One Product, One Term – Only assign a single Term to your product. All GMDN Terms are mutually exclusive. Multipurpose devices should be assigned to a Term describing a multipurpose device. Kits should be assigned to the appropriate kit Term. For implants, a set containing the implant is typically covered by the Term describing the implant. The definitions will indicate this.

Accurate Product Representation – Make sure the GMDN Term name and definition accurately represent your device. If key intended uses of your device are not mentioned in the definition, it may not be the appropriate Term.

Be Component Specific – A component of a system should be assigned to a Term that describes that component, not assigned to the Term for the overall system. Likewise, a component/accessory of a parent device should be assigned to a Term that describes that component/accessory, not assigned to the Term for the Parent device.